

**Programmed Sampling for
Screening Airborne Aerosols**

- Small, lightweight, compact
- Easy to use
- Accepts *BUCK* Impaction-Gel Slides or generic greased slides
- Battery powered, recharge or operate with Included Charger/ Adapter
- Five hour* run time at 15 LPM
- Optional *FastOne™* Charger (provides full charge in one hour)
- End-of-cycle and Battery Level audible & visual
- Tripod mount for area sampling

*Depends on battery maintenance, backpressure, etc.



*Controlled Flow Sampling Pump
for Gel-Impaction Slides*

The *BUCK BioSlide™* Model B1020 Sampling Pump is a compact, lightweight 10-20 LPM controlled flow sampling pump for bioaerosol sampling with *BUCK* Impaction-Gel (also accommodates generic grease slides). The easy, full-control keypad lets you perform unattended time programmed (1, 2, 5, or 10 minute) samples, perform easy calibrations without tools, or perform manual timed sampling at the touch of a button. A group of status LEDs show the *BUCK BioSlide™* Model B1020 operation at a glance. Both an LED and audible alarm provide confirmation of end-of-sample or depleted battery. The *BUCK BioSlide™* Model B1020 Pump provides a full five hours of continuous operation (at 15 LPM) from its rechargeable NiCad batteries. It comes with a Calibrated Rotameter for quick flow check or calibration and a Standard Charger. An optional *FastOne™* one-hour charger provides the ultimate in power management and time savings.

PRODUCT	DESCRIPTION
APB-707000	<i>BUCK BioSlide™</i> Pump Model B1020, complete with standard 120 VAC adapter/charger, instruction manual, and APB-706100 Calibration Rotameter Assembly.
APB-707020	<i>BUCK BioSlide™</i> Pump Model B1020, complete with standard 230 VAC adapter/charger, instruction manual, and APB-706100 Calibration Rotameter Assembly.
APB-601900	<i>FastOne™</i> Charger, 100-240VAC, provides on-hour battery charge, optional
APB-108010	Standard Charger, 120VAC
APB-108012	Standard Charger, 230 VAC
APB-706200	Calibration Rotameter Assembly, fits onto top of gel-impaction slide case
SAM-500910	<i>BUCK</i> Gel-Impaction Slide, shelf life one year from mfg. date, box 10

Rev. 01-2006

BUCK BioSlide™ Model B1020 Operation

The *BUCK BioSlide™* pump, Model B1020, provides a selectable, continuous, constant sample flowrate and is simple to operate. No tools are required. Its quiet operation allows unobtrusive sampling in IAQ, medical, clean room, public and residential building applications.

The front key pad is organized into three functional key groups: **Power** (ON-OFF), **Timing** (1, 2, 5, 10 minute samples), and **Calibration** (Cal mode, Increase flow, Decrease flow). Positive tactile feedback is provided by the keys. The *BUCK BioSlide™* Pump has internal NiCad batteries to provide a full five hours continuous run time at 15 LPM. The standard charger provides a battery recharge in 12-16 hours and allows the unit to operate on AC power; the optional FastOne™ Charger provides a battery recharge in one hour.

End of sample notice is provided by the lit LED "Complete" and three short beeps.

BUCK BioSlide™ Model B1020 Sampling Steps

Before sampling, ensure the battery is fully charged and that the "Low Battery" LED is not on. For greatest accuracy, the pump should be calibrated once a day.

1. Place pump in desired location.
2. Immediately before sampling, open a Buck BioSlide and log the serial number on a work sheet.
3. Open the pump slide door and place the microscope slide (with impact gel up) down into the recessed slot in the bottom of the pump. Close the top and check to assure the top is closed tightly.
4. Push the "ON" button to power up the *Buck BioSlide™* Pump and either: (a) continue to hold the "ON" button for four seconds to put pump in "Continuous" mode, or (b) push one of the programmed time keys (1, 2, 5, or 10 minutes) for an automatic timed sample.
5. At the end of programmed sample period, pump will automatically shut off and "Complete" LED will be lit; under "Continuous" mode, push and hold "OFF" button for 2 seconds to shut off pump.
6. Open and remove the slide by grasping at end where the serialized number are located.
7. Replace in its original box and send to an appropriate laboratory for analysis.

Specifications: Model B1020

Flowrate: 10—20 LPM constant flow


Accuracy: ± 5% of set point


Run Time: 10 LPM: 9 hrs, 15 LPM: 5 hrs,
20 LPM: 3.5 hrs

Size: 4" H x 6" W x 5¼" D
(10.2 cm H x 15.2 cm W x 13.3 cm D)

Weight: 29 oz. (826 g)

Compatibility: *BUCK* Gel-Impaction Slide

 * Prices and Specifications subject to change without notice.

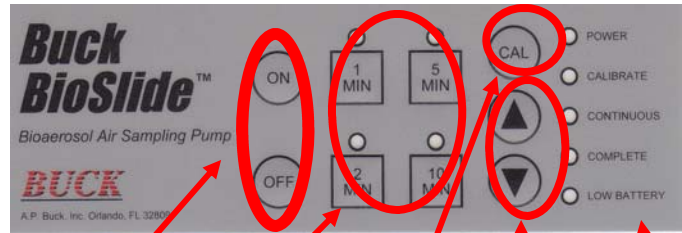

Power on.
Hold ON 4 sec to put *BioSlide™* into "Continuous" Mode. Hold OFF for 2 seconds to shut pump down

Push one of fixed sample time buttons after Power "ON"
Calibration Mode

Flow Adjust (in Cal Mode) up or down
Status LEDs confirm all pump functions

BioSlide™ Model B1020 Calibration

For greatest accuracy, the *BioSlide™* Model B1020 Pump should be calibrated once per day. Calibration is performed with an actual *BUCK* Gel-Impaction Slide installed. The *BUCK BioSlide™* Model B1020 Pump is a controlled flow device specially designed to accommodate the natural backpressure inherent in Gel-Impaction Slide. It is for use only with microscope slides 1X3 inches in size.

1. Place the flowmeter over the inlet of the BioSlide pump. The built in o-ring seal of the rotometer will give a tight connection.
2. Push "ON", then press the "CAL" for 2 seconds to put pump into calibration mode. Adjust the flowrate using the ▲ and ▼ keys to set center of rotometer ball to the desired flow rate mark on rotometer. Fine adjustments are possible. Allow pump to stabilize.
3. When flowrate is achieved, push "CAL" to accept setting, then turn pump off.
4. Verify the flow at anytime with the rotometer by selecting a 1,2,5 or 10 minute timing routing. Press the OFF key to stop. If the verify flow was accurate entering Cal is not necessary. Entering the Cal mode removes the previous setting for a new flow rate.



BUCK BioSlide™ Model B1020 Pump is shown with *BUCK* Gel-Impaction Slide and APB-706200 Calibration Rotometer Assembly

Rev. 01-2006

Calibration of the *BUCK BioSlide™* Model B1020 Pump is fast and easy. The supplied calibration Rotometer assembly fits securely on top of the Gel-Impaction Slide with no leakage, so all your sample airflow goes through the Gel-Impaction Slide. Flow calibration with an actual slide in-line ensures an accurate and repeatable calibration, without substitute restrictors, bubble tubes, or other fittings.