

Keysight N2797A Extreme Temperature Single-Ended Active Probe

User's
Guide



Notices

© Keysight Technologies, Inc. 2013 - 2014, 2018

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, Inc. as governed by United States and international copyright laws.

Manual Part Number

N2797-97001

Edition

Third edition, October 2018

Published by:
Keysight Technologies, Inc.
1900 Garden of the Gods Road
Colorado Springs, CO 80907 USA

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

U.S. Government Rights

The Software is "commercial computer software," as defined by Federal Acquisition Regulation ("FAR") 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement ("DFARS") 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at <http://www.keysight.com/find/sweula>. The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight:

(1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No additional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect

to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFAR 227.7103-5 (c), as applicable in any technical data. 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

Contents

1	Using the Probe / 5
	Probe Features / 7
	Using the Accessory Tips and Grounds / 14
	Dynamic Range and Offset Voltage Limitations / 20
	Functional Test / 21
	Inspecting the Probe / 22
	Cleaning the Probe / 22
	Returning the Probe for Service / 23
	Safety Information / 24
2	Probe Calibration / 27
	Calibrating the Probe on Infiniium Oscilloscopes / 28
	Calibrating the Probe on InfiniiVision Oscilloscopes / 30
3	Characteristics and Specifications / 31
	Dimensions / 33
4	Performance Data Plots / 35
5	Performance Verification / 37
	Test 1. DC Input Resistance / 39
	Test 2. Bandwidth / 40
	Performance Test Record / 46
	Index

1 Using the Probe

Probe Features	7
Using the Accessory Tips and Grounds	14
Dynamic Range and Offset Voltage Limitations	20
Functional Test	21
Inspecting the Probe	22
Cleaning the Probe	22
Returning the Probe for Service	23
Safety Information	24

The N2797A single-ended active probe is designed to be used in extreme temperatures environments. With a 2 meter cable and ability to operate in temperatures from -40°C to $+85^{\circ}\text{C}$, the N2797A probe is ideal for environmental labs. The probe's bandwidth is 1.5 GHz.

The N2797A integrates many of the characteristics needed for today's general-purpose, high-speed probing, especially in digital system design, component design/characterization, and educational research applications. Its 1 $\text{M}\Omega$ input resistance and extremely low input capacitance (1 pF) provide ultra low loading of the device under test. This, accompanied with superior signal fidelity, makes this probe useful for most of today's digital logic voltages. With a wide $\pm 8\text{V}$ dynamic range and $\pm 12\text{V}$ offset range, this probe can be used in a wide variety of applications.

For high signal integrity probing, the N2797A 1.5 GHz active probe is a perfect complements to Keysight's 500 MHz – 600 MHz and 1 GHz bandwidth scopes.

The probe is powered directly by the InfiniiVision and Infiniium AutoProbe interface, eliminating the need for an additional power supply. The probe also come with a number of accessories that allow for easy connections to the circuit under test. Refer to "[Supplied Accessories](#)" on page 8.

WARNING

Handle the probe with care to avoid injury, especially when it is fitted with the sharp spring or rigid tip.

CAUTION

This probe is an ESD sensitive devices, particularly at the probe tips. Follow standard ESD precautions when handling. Remove tip accessories when storing the probe.

CAUTION

Before using the probe, refer to **"Safety Information"** on page 24.

CAUTION

Handle the probe cable carefully to avoid damaging it through excessive bending or pulling. Avoid any mechanical shocks to the probe in order to guarantee accurate performance and protection.

Probe Features

Oscilloscope Compatibility

The N2797A probe is compatible with the Keysight oscilloscopes shown in [Table 1](#). Up to four probes can be connected to the oscilloscope. The table also lists the minimum required firmware version for the oscilloscope.

NOTE

The N2797A probe is designed for oscilloscopes with 1 MΩ AutoProbe-interface channel inputs.

Is Your Oscilloscope Software Up-to-Date? Keysight periodically releases software updates to support your probe, fix known defects, and incorporate product enhancements. To download the latest firmware, go to www.keysight.com and search for your oscilloscope’s topic. Click on the “Drivers, Firmware & Software” tab.

Table 1 Compatible Oscilloscopes and Support

Oscilloscope	Adapter Required
Infiniium Oscilloscopes (<i>firmware version ≥ 3.50 or above</i>)	
90000 Q-Series	N5442A
90000 X-Series	N5442A
90000A	—
9000 H-Series	—
9000A-Series	—
InfiniiVision Oscilloscopes (<i>firmware version ≥ 2.11 or above</i>)	
4000 X-Series	—
3000 X-Series	—

Probe Headlight

The probe is equipped with a white LED headlights to illuminate the area around the probe tip. This headlight has a fixed intensity and is turned on and off by pressing the button that is located on the probe's body.

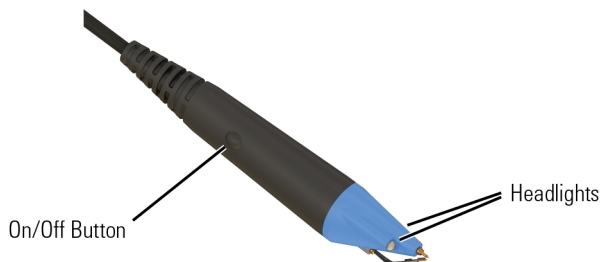


Figure 1 Headlights and Button

Channel-Identification Rings

When multiple probes are connected to the oscilloscope, the channel identification rings (yellow, green, blue, and purple) allow you to quickly determine which channel input is associated with each probe. On the probe, place one colored ring near the probe's channel connector and place an identical color ring near the probe head.

Supplied Accessories

The probe comes with the accessories shown in [Figure 2](#).

CAUTION

All of the supplied accessories can be used at the probe's specified extreme temperature range of -40°C to $+85^{\circ}\text{C}$ (-40°F to $+185^{\circ}\text{F}$) except the flex nose clip and pico hook tips. These adapters have a slightly reduced temperature range of -20°C to $+80^{\circ}\text{C}$ (-4°F to $+176^{\circ}\text{F}$).

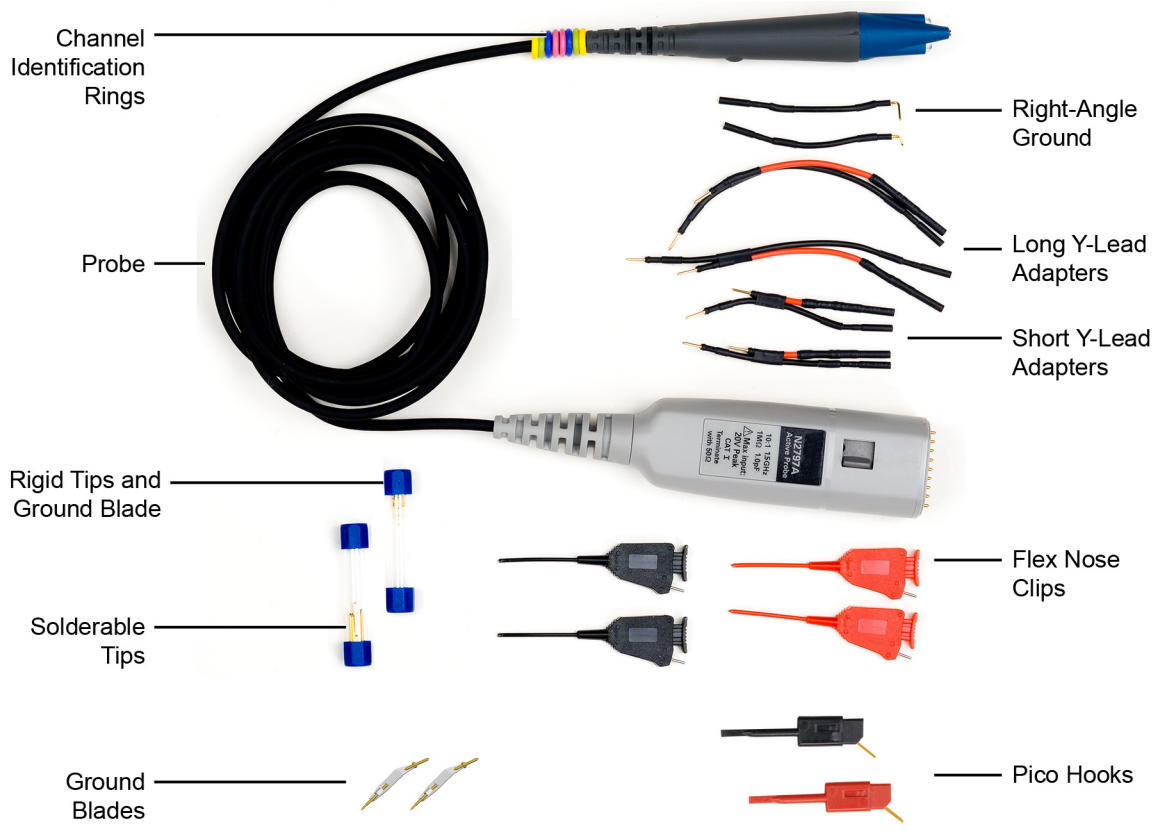


Figure 2 Accessories Supplied With the Probe (Not to Scale)

Table 2 Supplied Accessories

Accessory	Ambient Operating Temperature	Quantity
Flex Nose Clip (red)	-20°C to +80°C (-4°F to +176°F)	2
Flex Nose Clip (black)		2
Pico Hook (red)		1
Pico Hook (black)		1
Rigid Probe Tip	Same as probe -20°C to +85°C (-4°F to +185°F)	5
Solderable Tip (0.97 mm square)		10
Ground Blade		2
Y-Lead Adapter, long with damping resistor (9 cm)		2
Y-Lead Adapter, short with damping resistor (6 cm)		2
Right-Angle Ground (5 cm)		2

Available Accessories

Table 3 shows the replacement accessories available in the N2798A replacement accessory kit. The table lists the ambient operating temperatures for each accessory. Those accessories that have the same temperature range as the probe are marked “*extreme temp*”.

Table 4 shows additional accessories that work with the probe, but are not provided with the probe. Notice that most of these accessories can not be used at extreme temperature range of the probe.

Table 3 Replacement Accessory Kit (N2798A)











Item	Description	Ambient Operating Temperature	Qty	Kit Part Number
	Solderable Tip, <i>extreme temp</i>	Same as probe –40°C to +85°C (–40°F to +185°F)	10	5061-7385
	Ground Blade, <i>extreme temp</i>		2	5061-7393
	Rigid Probe Tip, <i>extreme temp</i>		5	5061-7389
	Flex Nose Clips This adapter has a <i>slightly reduced</i> temperature range compared to the probe.	–20°C to +80°C (–4°F to +176°F)	2 (red) 2 (black)	5061-7390 (red) 5061-7391 (black)
	Pico Hook Nose Clips This adapter has a <i>slightly reduced</i> temperature range compared to the probe.	–20°C to +80°C (–4°F to +176°F)	1 (red) 1 (black)	–
	Long Y-Lead Adapter with damping resistor (10 cm), <i>extreme temp</i>	Same as probe –20°C to +85°C (–4°F to +185°F)	2	5061-7386
	Short Y-Lead Adapter with damping resistor (5 cm), <i>extreme temp</i>		2	5061-7387
	Right Angle Ground (5 cm), <i>extreme temp</i>	Same as probe –40°C to +85°C (–40°F to +185°F)	2	5061-7384

Table 4 Additional Available Accessories

Item	Description	Ambient Operating Temperature	Qty	Kit Part Number
	Spring Probe Tip, <i>extreme temp</i>		2	5061-7388
	Long Y-Lead Adapter(10 cm)	0°C to 50°C (32°F to 122°F)	1	5061-7392
	Right Angle Ground (10 cm)	0°C to 50°C (32°F to 122°F)	2	5061-7400
	Right Angle Ground (5 cm)		2	5061-7399
	Ground Lead (6 cm)	0°C to 50°C (32°F to 122°F)	2	5061-7395
	Ground Lead (12 cm)		2	5061-7396
	Offset Ground	0°C to 50°C (32°F to 122°F)	2	5061-7394
	N2787A 3D Probe Positioner	Not Specified	—	—

Attaching Probe Accessories

It's easy to change the probe tip and ground accessories. **Figure 3** shows locations for inserting the tip and the ground accessory. To change an accessory, gently pull it straight out of its contact socket along the axis of the probe. Once the accessory is removed, insert the new accessory until it is seated in the contact socket. In order to insert the probe tip completely into the housing, carefully press the probe tip against a hard surface.









Figure 3 Tip and Grounding Connections


Using the Accessory Tips and Grounds


This section presents the various probe accessory configurations listed in order of available bandwidth for your measurements. Select the configuration to match your measurement needs, including ease of use.

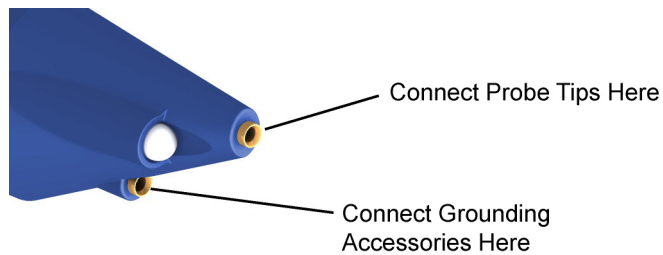Table 5 Probe Configuration in Order of Decreasing Bandwidth

Recommended Order of Use	Probe Configuration Topic	Typical Bandwidth
1	 "Rigid or Solderable Tip with Ground Blade" on page 15	1.5 GHz
2	 "6 cm Y-Leads with 0.1 inch Headers" on page 16	1.0 GHz
3	 "Solderable Tip with Right-Angle Ground" on page 17	800 MHz
4	 "9 cm Y-Leads with 0.1 inch Headers" on page 18	800 MHz
5	 "Y-Lead with Flexible Nose Clips and Pico Hooks" on page 19	500 MHz

Rigid or Solderable Tip *with* Ground Blade

 The combination of rigid or solderable tip and ground blade provide the highest bandwidth of any combination of accessory tips and grounds. Use this configuration at room temperatures where hand probing is possible or at extreme temperatures when using a probe positioner that can withstand the required temperature. The bandwidth with accessory is 1.5 GHz.

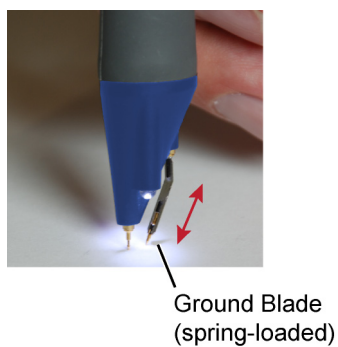

WARNING Handle the probe with care to avoid injury, especially when it is fitted with the sharp rigid or spring tip.

When inserting the tip, insert the end with the ridge into the probe head as shown in [Figure 4](#).


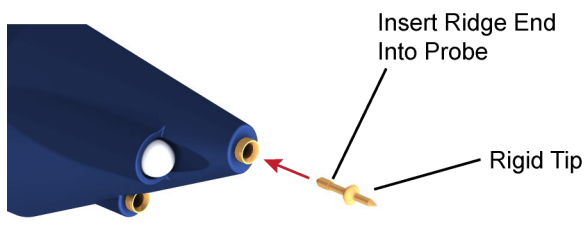


Figure 4 Inserting the Rigid Tip

6 cm Y-Leads with 0.1" Headers



The short 6 cm long Y-leads offer a convenient and reliable method to connect both the probe signal and ground to probe points on the board via or the solderable pins that are provided with each probe. The sockets accept 0.56 to 0.86 mm round and 0.64 mm square (0.022 to 0.034 inch round and 0.025 inch square) diameter pins. The maximum insertion depth is 7.5 mm (0.295 inch) and the outer insulation of the socket is less than

2.54 mm. You can use it for 2.54 mm pitch (0.1 inch) terminals. The bandwidth with accessory is 1.0 GHz.

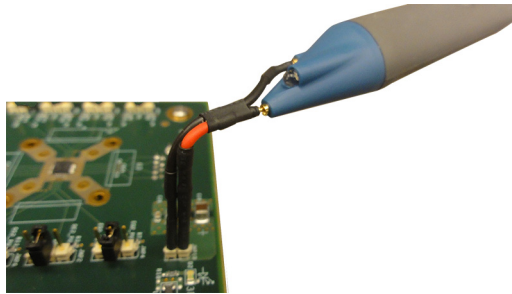


Figure 5 Probe with Y-Leads Attached

Solderable Tip *with* Right-Angle Ground



The solderable pin and right-angle ground provide hands free probing at extreme temperatures. Solder the tip on the printed-circuit board as shown in [Figure 6](#) and then slip the probe onto the free end of the solderable pin. The bandwidth with accessory is 800 MHz.

NOTE

The longer right-angle ground lead introduces increased inductance in the ground path. Therefore, keep the right-angle ground lead as straight as possible for maximum measurement bandwidth. Loops and bends in the ground lead, as shown in this picture, can reduce the measurement bandwidth.

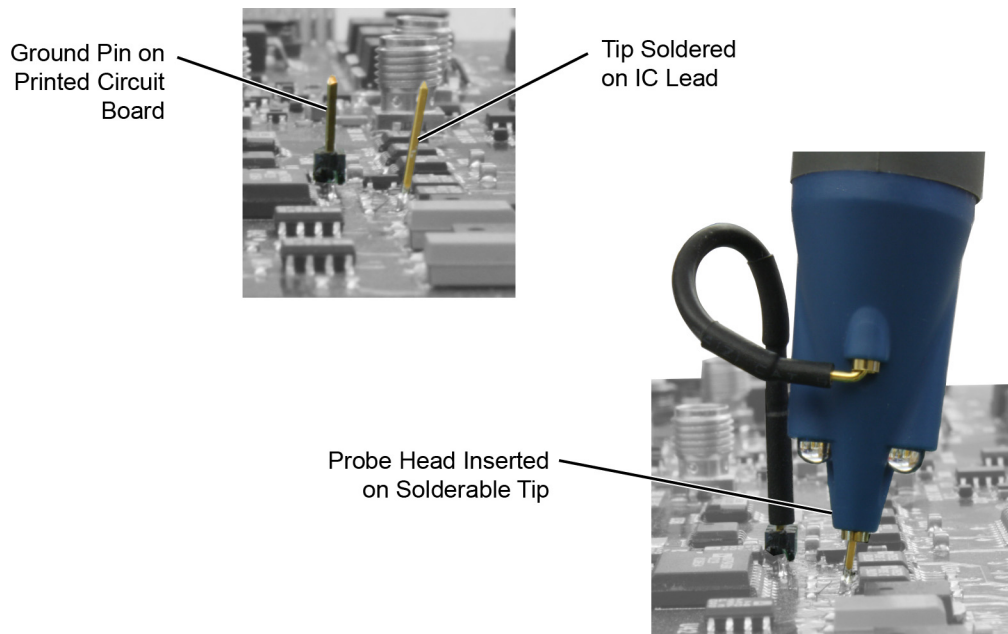


Figure 6 Placing the Probe Onto the Solderable Tip

9 cm Y-Leads with 0.1" Headers



Like the 6 cm Y-leads, the 9 cm Y-leads offer a convenient and reliable method to connect both the probe signal and ground to probe points on the board via or the solderable pins that are provided with each probe. The added convenience of the longer leads results in a slightly reduced bandwidth. The bandwidth with accessory is 800 MHz.

The sockets accept 0.56 to 0.86 mm round and 0.64 mm square (0.022 to 0.034 inch round and 0.025 inch square) diameter pins. The maximum insertion depth is 7.5 mm (0.295 inch) and the outer insulation of the socket is less than 2.54 mm. You can use it for 2.54 mm pitch (0.1 inch) terminals.

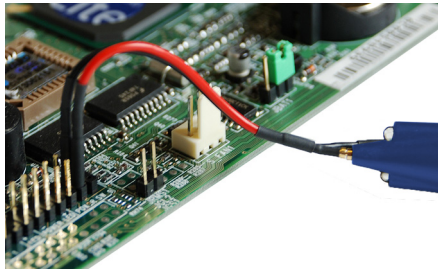


Figure 7 Probe with Y-Leads Attached

Y-Lead with Flexible Nose Clips and Pico Hooks

You can use flexible nose clips and Pico hook clips to make connections to components or wires with leads that are 1.01 mm (0.04 inches) in diameter or smaller. With today's miniature IC- and component-packaging techniques, these clips can make probing challenging devices much easier. The bandwidth with accessory is 500 MHz.

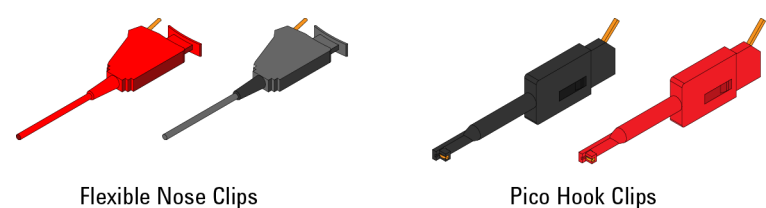


Figure 8 Flexible Nose and Pico Hook Clips

Most users prefer to attach the clips to the probe via the Y-lead adapter as shown in the picture below. Press the back of the clip to extend the grasping hook and then release to tighten the hook around the component you are testing.

CAUTION

The clips have an ambient operating temperature range of -20°C to +80°C (-4°F to +176°F). This is a slightly reduced range compared to the probe.

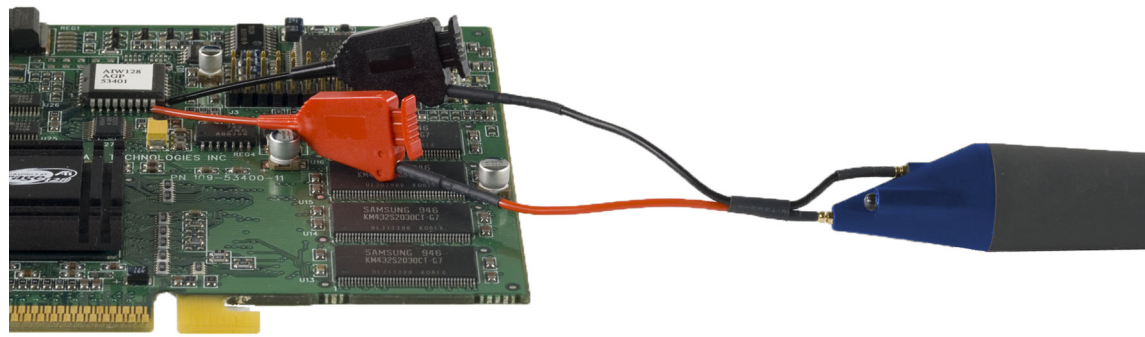


Figure 9 Probe with Flexible Nose Clips Attached



Dynamic Range and Offset Voltage Limitations

With the $16V_{pp}$ ($\pm 8V$) of dynamic range and $\pm 12V$ of offset range, the probes have a wide measuring range of $\pm 20V$ peak (mains isolated), which allows them to be used for a wide variety of applications. For example, if you wanted to measure small AC noise riding on top of a $+10V$ DC signal, you could use DC offset to position the signal at the center of the screen to keep the probe within its dynamic range. You could then zoom in to see the detail at a higher resolution. Trying to measure a signal out of the dynamic range may result in a clipped or distorted waveform.

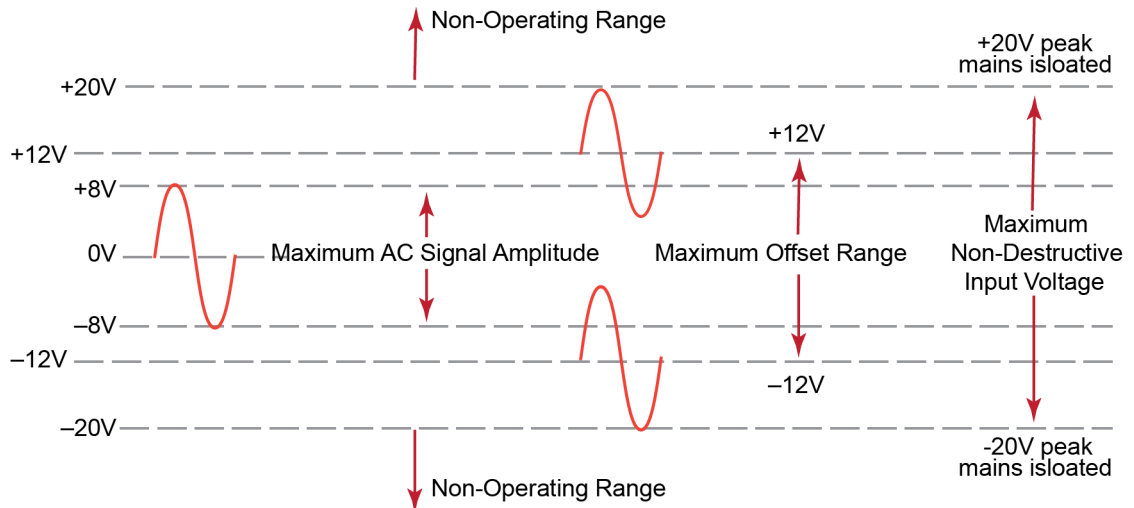


Figure 10 Dynamic Range and Offset Limits (mains isolated)

Functional Test

Use the following generic measurement procedure to ensure that your probe is functioning properly.

- 1** Connect the probe to an oscilloscope channel input and ensure the input impedance of the oscilloscope matches the output impedance of the probe (50Ω).
- 2** Connect a grounding accessory to the probe and connect the ground to the ground terminal on the oscilloscope.
- 3** Connect the probe tip to the oscilloscope's probe compensation output.
- 4** Enable autoscale on the oscilloscope.
- 5** A square wave should now be displayed on the oscilloscope, if the probe is functioning properly.

Inspecting the Probe

- Inspect the shipping container for damage.

Keep the damaged shipping container or cushioning material until the contents of the shipment have been checked for completeness and the probe has been checked mechanically and electrically.

- Check the accessories.
- If the contents are incomplete or damaged, notify your Keysight Technologies Sales Office.
- Inspect the probe.

If there is mechanical damage or defect, or if the probe does not operate properly or pass calibration tests, notify your Keysight Technologies Sales Office.

If the shipping container is damaged, or the cushioning materials show signs of stress, notify the carrier as well as your Keysight Technologies Sales Office. Keep the shipping materials for the carrier's inspection. The Keysight Technologies office will arrange for repair or replacement at Keysight Technologies' option without waiting for claim settlement.

Cleaning the Probe

Disconnect the probe from the oscilloscope and clean the probe with a soft cloth dampened with a mild soap and water solution. Make sure the probe is completely dry before reconnecting it to an oscilloscope.

Returning the Probe for Service

If the probe is found to be defective we recommend sending it to an authorized service center for all repair and calibration needs. Perform the following steps before shipping the probe back to Keysight Technologies for service.

- 1** Contact your nearest Keysight sales office for information on obtaining an RMA number and return address.
- 2** Write the following information on a tag and attach it to the malfunctioning equipment.
 - Name and address of owner
 - Product model number (for example, N2797A)
 - Product Serial Number (for example, MYXXXXXXXX)
 - Description of failure or service required

NOTE

Include probing and browsing tips if you feel the probe is not meeting performance specifications or a yearly calibration is requested.

- 3** Protect the probe by wrapping in plastic or heavy paper.
- 4** Pack the probe in the original carrying case or if not available use bubble wrap or packing peanuts.
- 5** Place securely in sealed shipping container and mark container as "FRAGILE".

NOTE

If any correspondence is required, refer to the product by serial number and model number.

Contacting Keysight Technologies

For technical assistance, contact your local Keysight Call Center.

- In the Americas, call 1 (800) 829-4444
- In other regions, visit <http://www.keysight.com/find/assist>

Before returning an instrument for service, you must first call the Call Center at 1 (800) 829-4444.

Safety Information

To avoid personal injury and to prevent fire or damage to this product or products connected to it, review and comply with the following safety precautions. Be aware that if you use this probe assembly in a manner not specified, the protection this product provides may be impaired.

WARNING

Handle the probe with care to avoid injury, especially when it is fitted with the sharp spring or rigid tip.

WARNING

Handle Probe Tips and Accessories Carefully. Some of the probe tips and accessories are very sharp (the browser tips, for example). You should handle these with care to avoid personal injury.

WARNING

Use Only Grounded Instruments. Do not connect the probe's ground lead to a potential other than earth ground. Always make sure the probe and the oscilloscope are grounded properly.

WARNING

Connect and Disconnect Properly. Connect the probe to the oscilloscope and connect the ground lead to earth ground before connecting the probe to the circuit under test. Disconnect the probe input and the probe ground lead from the circuit under test before disconnecting the probe from the oscilloscope.

WARNING

Observe Probe Ratings. Do not apply any electrical potential to the probe input which exceeds the maximum rating of the probe. Make sure to comply with the voltage versus frequency derating curve found in this manual.

The probe should NOT be used to make measurements on mains circuits (CAT II, CAT III, CAT IV).

WARNING


Keep Away From Live Circuits. Avoid open circuitry. Do not touch connections or components when power is present.

- WARNING

Indoor Use Only. Do not operate in wet/damp environments. Keep product surfaces dry and clean.
-
- WARNING

Service should be carried out by a Keysight Technologies authorized service personnel. For any service needs, contact Keysight Technologies. Refer to the topic **“Returning the Probe for Service”** on page 23 to know more.
-
- CAUTION


The probe cable is a sensitive part of the probe and, therefore, you should be careful not to damage it through excessive bending or pulling. Avoid any mechanical shocks to this product in order to guarantee accurate performance and protection.
-
- WARNING






These probes are for use only on mains isolated circuits. These are NOT intended for measurements on CAT II, CAT III, or CAT IV circuits.
-
- WARNING

Periodically inspect the probe and cable. Do not use a probe which is cracked, damaged, or has defective leads. If a failure is suspected, do not use the probe. Contact Keysight Technologies for technical assistance.
-

Instrument Markings

Symbol	Description
	The CE mark is a registered trademark of the European Community. ISM GRP 1-A denotes the instrument is an Industrial Scientific and Medical Group 1 Class A product. ICES/NMB-001 indicates product compliance with the Canadian Interference-Causing Equipment Standard.

Symbol	Description
	This product complies with the WEEE Directive (2002/96/EC) marking requirements. The affixed label indicates that you must not discard this electrical/electronic product in domestic household waste. Product Category: With reference to the equipment types in the WEEE Directive Annex I, this product is classed as a “Monitoring and Control instrumentation” product. Do not dispose in domestic household. To return unwanted products, contact your local Keysight office, or refer to www.keysight.com for more information.
	This symbol indicates the Environmental Protection Use Period (EPUP) for the product's toxic substances for the China RoHS requirements.
	Instruction manual symbol: The product is marked with this symbol when it is necessary for you to refer to the instruction manual in order to protect against damage to the product or personal injury.

2 Probe Calibration

Calibrating the Probe on Infiniium Oscilloscopes **28**
Calibrating the Probe on InfiniiVision Oscilloscopes **30**

Always calibrate the probe before making any critical measurements. A probe calibration removes attenuation errors, offset errors, and timing delays that are introduced by the probe. This chapter contains basic calibration procedures for both Infiniium and InfiniiVision oscilloscopes. For additional information on the probe calibration refer to the oscilloscope's user documentation.

CAUTION

Always wear an ESD wrist strap when working with active probes. Not doing so can result in the probe becoming permanently damaged.

Calibrating the Probe on Infiniium Oscilloscopes

Probe calibrations vary slightly between series 9000, 90000, and 90000 X oscilloscopes. For 9000 series oscilloscopes, the following calibrations are used:

- Skew Calibration
- Attenuation/Offset Calibration

For 90000 series oscilloscopes, the following calibrations are used:

- DC Attenuation/Offset Calibration
- Skew Calibration

When performing a the skew calibration, the E2655B Performance Verification (PV) and deskew fixture is used. The PV fixture is included with the Deskew Kit which is shipped with Infiniium oscilloscopes. The fixture is also used in the performance verification procedure that is documented in [Chapter 5](#), “Performance Verification”.

An optional N2787A 3D Probe Positioner or equivalent can be used to hold the probe during the calibration.



Procedure

- 1 Turn on the oscilloscope. Allow the oscilloscope and probe to warm up for 20 minutes before performing the probe calibrations.
- 2 If the oscilloscope needs calibration, perform a user calibration before the probe calibration. On the oscilloscope, click **Utilities > Calibration**.
- 3 On the oscilloscope, click **Setup > Probes**.
- 4 In the Probe Calibration dialog box, select the tab representing the channel that has the probe attached.
- 5 In the dialog box, select the probe head and the type of calibration. Click **Start** and follow the instructions shown on the oscilloscope.
- 6 When performing the skew calibration, you will be instructed to use the PV fixture. Observe these points:
 - Connect the PV fixture's input to the oscilloscope's calibration output as shown in [Figure 11](#) on page 29. Connect a 50 ohm terminator to the PV's output.

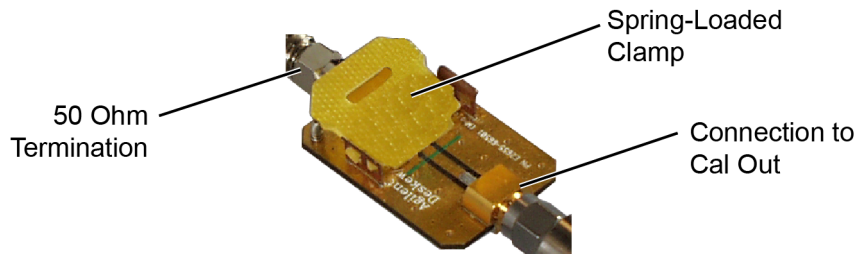


Figure 11 E2655B PV Fixture with 50 Ohm Termination

- Position the probe so that the signal lead touches the PV fixture's center conductor next to the dielectric area. The ground lead should touch the PV fixture's ground plane. On 90000 X-series oscilloscopes, use an N5442A adapter when instructed to connect the probe to one of the oscilloscope's channel inputs.

CAUTION

To avoid damaging the oscilloscope's **Cal Out** connector, do not apply force to the PV fixture. Light probe contact is all that is needed for the calibration.

CAUTION

NEVER solder a probe tip to the thick-film gold. The gold will immediately dissolve into the solder and disappear.

NOTE

If you are using the browser tip, it is recommended that you use the N2787A 3D Probe Positioner to hold the probe in place.

NOTE

You can check that the probe leads are correctly connected by pressing the front panel autoscale button. A stable step should be shown on the screen. Pressing autoscale will close the Probe Calibration dialog box.

Calibrating the Probe on InfiniiVision Oscilloscopes

Allow the oscilloscope and probe to warm up for 20 minutes before performing the probe calibration.

Procedure

- 1 Connect the probe to one of the oscilloscope channels.

NOTE

When you connect the probe, the **Calibrate Probe** softkey in the Channel Probe Menu becomes active.

- 2 Connect the probe to the calibration terminals. On 3000 X-series oscilloscopes, connect the probe's signal tip to the front-panel **Demo 2 / Probe Comp** terminal and the ground tip to the ground terminal.

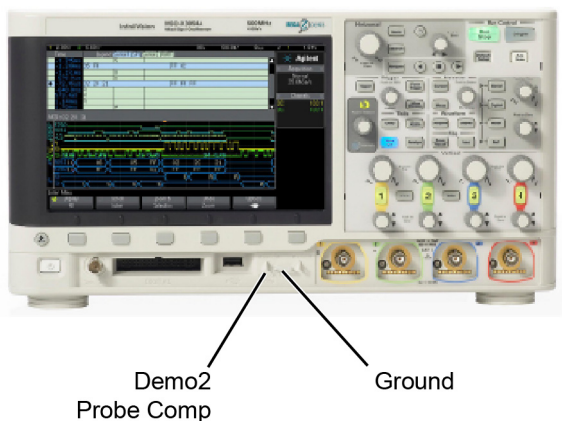


Figure 12 Probe Calibration Terminals on 3000 X-Series Oscilloscope

- 3 Press the Channel on/off key to turn the channel on (if the channel is off).
- 4 In the Channel Menu, press the **Probe** softkey.
- 5 Press the **Calibrate Probe** softkey and follow the instructions on the display.

3 Characteristics and Specifications

This chapter provides the characteristics and specifications for the N2797A active probe. The probe and oscilloscope should be warmed up for at least 20 minutes before any testing and the environmental conditions should not exceed the probe's specified limits.

Table 6 Mechanical Characteristics

Parameter	Characteristic
Probe Weight	108g (approximate)
Cable Length	2m

Table 7 Environmental Specifications


Parameter	Characteristic
Ambient Operating Temperature	-40°C to +85°C (-40°F to +185°F) Operating: -10 °C to +55 °C (probe pod) Non-operating: -40 °C to +70 °C (probe pod)
Ambient Non-Operating Temperature	-40°C to +85°C (-40°F to +185°F)
Operating Humidity	95% RH at +40°C (non-condensing)
Non-Operating Humidity	95% RH at +65°C
Operating Altitude	4,000m (13,000 ft)
ESD	8 kV HBM

Table 8 Electrical Characteristics and Specifications

Parameter	Characteristic or Specification (<i>where indicated</i>)
Bandwidth (–3 dB) ^a	1.5 GHz (<i>specification</i>)
Rise Time (10% – 90%, calculated)	233 ps
System Bandwidth (with Keysight oscilloscope)	1 GHz (with Keysight's 1 GHz InfiniiVision or Infiniium oscilloscope)
Attenuation Ratio (at DC)	10:1 ± 0.5%
Input Dynamic Range	–8V to +8V (DC or Peak AC) (mains isolated)
Non-Destructive Maximum Input Voltage	–20V to +20V (mains isolated)
Offset Range	±12V
DC Offset Error (Output Zero)	< ±1 mV
Flatness (at 25° C)	Typical 0.3 dB (10 Hz – 100 MHz) Typical 0.8 dB (100 MHz – 1 GHz) Typical 2.0 dB (1 GHz – 1.5 GHz)
Flatness Over Temperature (–40° C to +85° C)	Typical 0.3 dB (10 Hz – 100 kHz) Typical 0.6 dB (100 kHz – 100 MHz) Typical 0.8 dB (100 MHz – 500 MHz) Typical 2.0 dB (500 MHz – 1 GHz) Typical 2.5 dB (1 GHz – 1.5 GHz)
Input Resistance ^a	1 M Ω ± 3% (<i>specification</i>)
Input Capacitance	1 pF
Probe Noise	< 2.5 mV _{rms} (referred to input)
Output Impedance	50 Ω
Internal Power	Keysight AutoProbe interface from oscilloscope (InfiniiVision and Infiniium)

^a Denotes warranted electrical specification at 25 °C room temperature after 20 minute warm-up. All others are typical.

Dimensions

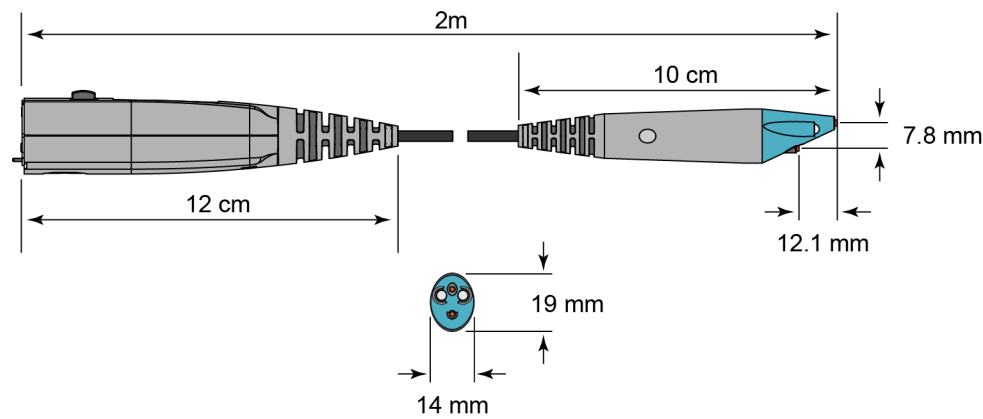

4 Performance Data Plots

Figure 13 shows the frequency response for the spring or rigid probe tip and an offset ground or ground blade.

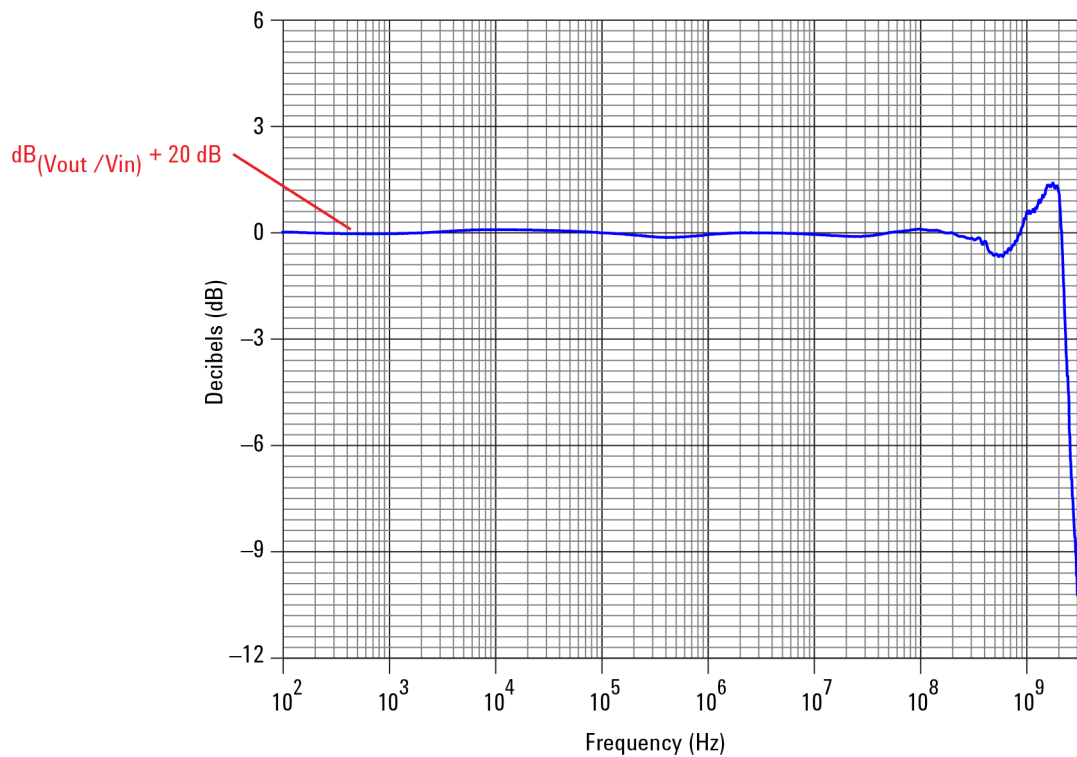


Figure 13 Frequency Response ($V_{\text{out}}/V_{\text{in}}$)

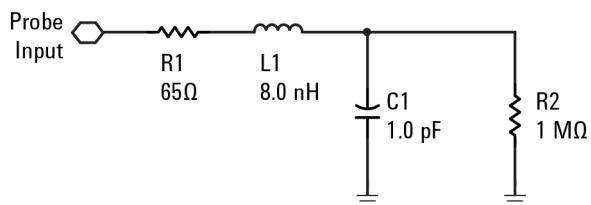


Figure 14 Input Impedance Equivalent Model

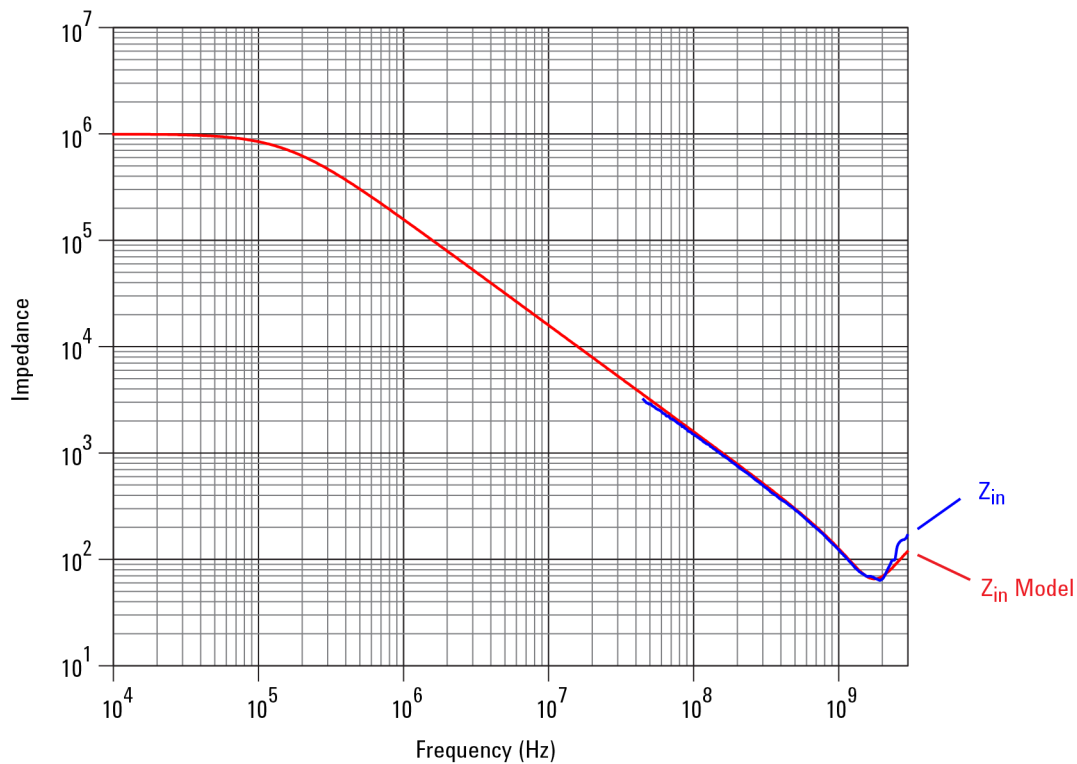


Figure 15 Typical Input Impedance Plot

5 Performance Verification

Test 1. DC Input Resistance 39

Test 2. Bandwidth 40





Performance Test Record 46

These procedures are used to test the warranted specifications for the N2797A. The recommended calibration test interval is once a year or as required. Use the equipment listed in [Table 9](#) on page 38.

CAUTION

Electrostatic discharge (ESD) can quickly and imperceptibly damage or destroy high performance probes, resulting in costly repairs. Always wear a wrist strap when handling probe components and insure that cables are discharged before being connected.

Table 9 Required Test Equipment

Test Equipment	Critical Specification	Model Number
Digital Multimeter (DMM)	Resistance $\pm 1\%$	Keysight 34401A
Vector Network Analyzer (VNA)	13 GHz sweep range full 2 port cal Option 1D5	Keysight 8720ES
		
Calibration Standards	No Substitute	Keysight 85052D
External Power Supply	No Substitute	Keysight 1143A
		
AutoProbe Interface Adapter	No Substitute	Keysight N1022A/B
		
Outside thread 3.5 mm (male) to 3.5 mm (female) adapter	No Substitute	Keysight 5062-1247
Cable (2)	3.5 mil; SMA; High Quality	Keysight 8120-4948
Cable	1.5 mil Probe Power Extension No Substitute	Keysight 01143-61602
PV/DS Test Board	No Substitute (In E2655B Kit)	Keysight E2655-66503
		

Test 1. DC Input Resistance

Procedure

- 1** Connect the DMM probes between the probe tip and ground at the tip of the probe.
- 2** Set up the DMM to measure resistance. The resistance should read $1\text{ M}\Omega \pm 3\%$.
- 3** Record the resistance in [Table 10](#) on page 46.

Test 2. Bandwidth

NOTE

Allow the probe to warm up for at least 20 minutes.

Using the 8720ES VNA successfully

Observe these simple guidelines when working with the 8720ES VNA during this procedure.

- Sometimes it may take a few seconds for the waveforms to settle completely. Allow time for waveforms to settle before continuing.
- Make sure all connections are tight and secure. If needed, use a vise to hold the cables and test board stable while making measurements.
- Be careful not to cross thread or force any connectors. This could be a very costly error to correct.

Procedure

Initial Setup

- 1 Turn on the 8720ES VNA and let warm up for 20 minutes.
- 2 Press the green **[Preset]** key on the 8720ES VNA.
- 3 On the VNA, press the **[Power]** key and set the power to 0 dBm.
- 4 On the VNA, press the **[AVG]** key and then select the **Averaging Factor** screen key. Set averaging to 4.
- 5 On the VNA, press the **[Sweep Setup]** key and then press the **sweep type menu** screen key. Select the **log freq** screen key.
- 6 Connect the probe under test to the AutoProbe Adapter and power the probe using the 1143A power supply as shown in **Figure 16** on page 41. Install the outside thread adapter to the AutoProbe Adapter.

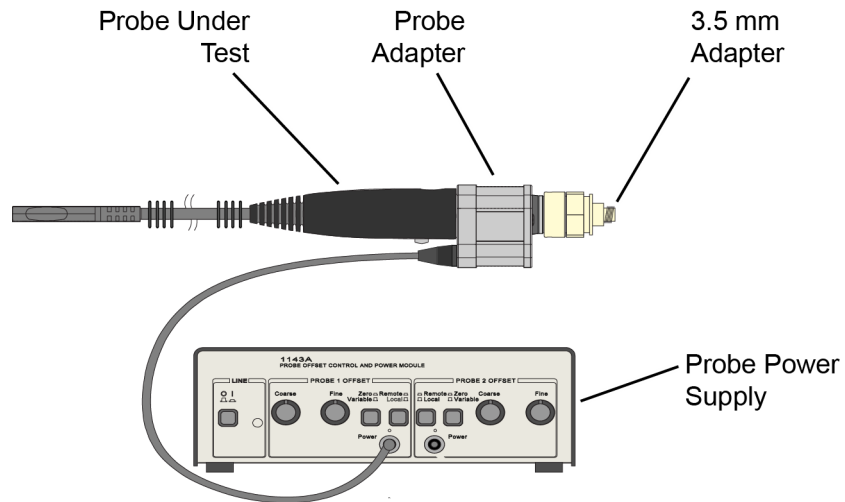


Figure 16 Probe Connected to Probe Adapter (*not to scale*)

Calibrating a Reference Plane

To get a reliable measurement from the VNA you must calibrate a reference plane so that the VNA knows where the probe under test is located along the transmission line.

- 7 On the VNA, press the **[Cal]** key.
- 8 Press the **cal menu** screen key.
- 9 Press the **full 2 port** screen key.
- 10 Connect the PV fixture to the **Port 1** on the VNA using a high quality SMA cables. Connect the cable to the pincher side of PV fixture as shown in [Figure 17](#) on page 42.
- 11 The calibration reference plane is at the other end of PV fixture.

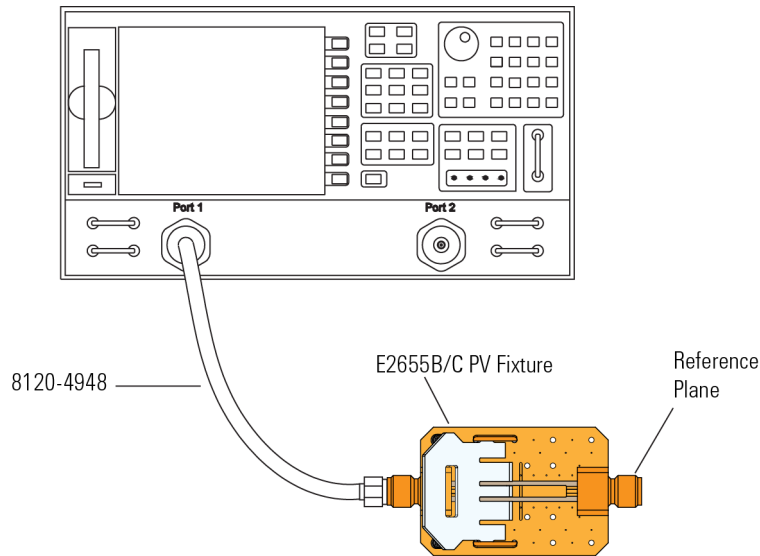


Figure 17 PV Fixture Connected to VNA

- 12 Perform a Calibration for the **PORT 1** side of the Reference plane.
 - a Press the **reflection** screen key.
 - b Connect the open end of 85052D Calibration Standard to the non-pincher side of the PV/DS test board.
 - c Select the **open** screen key under the **Forward** group.
 - d Wait until the VNA beeps indicating that it has completed the task.
 - e Connect short end of Calibration Standard to the non-pincher side of the PV/DS test board.
 - f Select **short** screen key under the **Forward** group.
 - g Wait until the VNA beeps indicating that it has completed the task.
 - h Connect load end of Calibration Standard to the non-pincher side of the PV/DS test board.
 - i Select the **loads** screen key under the **Forward** group.
 - j Press **broadband** screen key selection.
 - k Wait until the VNA beeps indicating that it has completed the task.
 - l Press the **done loads** screen key.
 - m You have just calibrated one side of the reference plane.
- 13 Connect the other high quality SMA cable to the VNA's **PORT 2** as shown in [Figure 18](#).

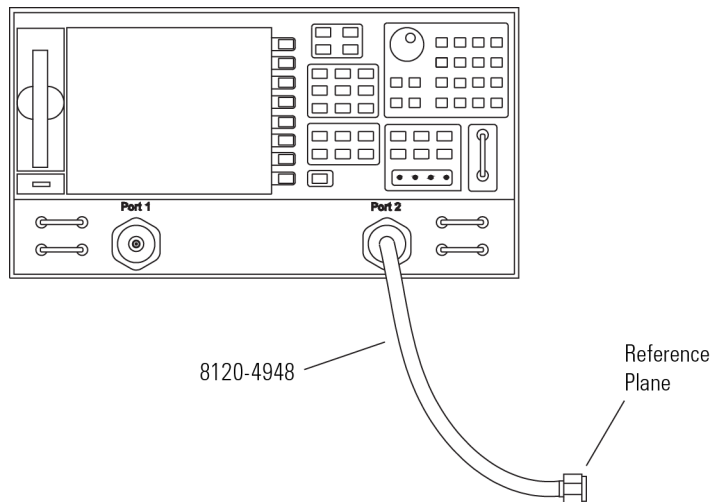


Figure 18 SMA Cable Connected to Port 2

- 14 Get the opposite sex of the Calibration Standards for the next step.
- 15 Perform Calibration for the **PORT 2** side of the Reference plane.
 - a Press the **reflection** screen key.
 - b Connect the open end of Calibration Standard to the available end of the **PORT 2** SMA cable.
 - c Select the **open** screen key under the **Reverse** group.
 - d Wait until the VNA beeps indicating that it has completed the task.
 - e Connect short end of Calibration Standard to the available end of the **PORT 2** SMA cable.
 - f Select **short** screen key the **Reverse** group.
 - g Wait until the VNA beeps indicating that it has completed the task.
 - h Connect load end of Calibration Standard to the available end of the **PORT 2** SMA cable.
 - i Select the **loads** screen key the **Reverse** group.
 - j Press **broadband** screen key selection.
 - k Wait until the VNA beeps indicating that it has completed the task.
 - l Press the **done loads** screen key.
 - m You have just calibrated the other side of the reference plane.
- 16 Press **standards done** key.
- 17 Connect the **PORT 2** SMA cable to the non-pincher side of PV fixture as shown in [Figure 19](#).

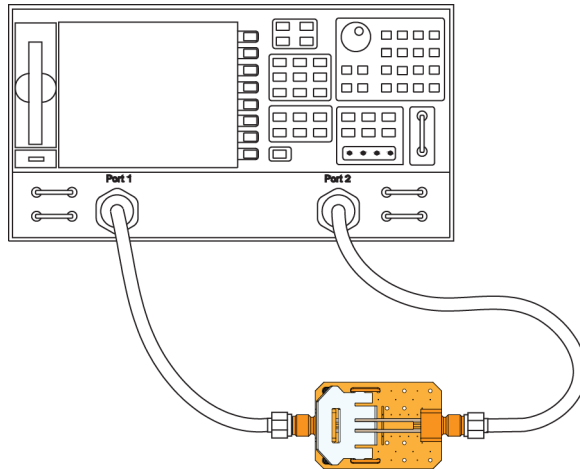


Figure 19 Forward and Reverse Setup

- 18 Press the **transmission** screen key.
- 19 Press the **do both fwd and reverse** screen key.
- 20 Wait until the VNA beeps four times indicating that it has completed the task.
- 21 Press the **isolation** screen key.
- 22 Press the **omit isolation** screen key.
- 23 Press **done 2 port cal** screen key.
- 24 Set the VNA's averaging to off.
- 25 Save the reference plane cal by pressing the **[save recall]** key then the **[save state]** key.
- 26 You may change name if you wish.
- 27 Press the **[scale reference]** key. Then set the scale to 1 dB per division and the reference position for 7 divisions.
- 28 Set reference value for 0 dB.
- 29 Press the **[measure]** key.
- 30 Press the **s21** screen key.
- 31 Ensure s21 response on screen is flat out to 1.5 GHz.

Measuring Vin Response

- 32 Position the probe conveniently to allow the probe tip to be normal to the PV/DS board.
- 33 Hold the probe in position, or use a positioner, so that the signal and ground are making contact and are perpendicular to the fixture.
- 34 Press the **[Sweep Setup]** key on the VNA. Then press the **trigger menu** screen key. Select the **continuous** screen key.
- 35 You should now have the V_{in} waveform on screen.
- 36 Select **[display]** key then **data->memory** screen key.
- 37 You have now saved Vin waveform into the VNA's memory for future use.

Measuring Vout Response

- 38 Disconnect the **PORT 2** cable from PV/DS test board and attach to probe output on the AutoProbe Adapter.
- 39 Connect the Calibration Standard load to PV/DS test board (non-pincher side).
- 40 Press **[scale reference]** key on the VNA.
- 41 Set reference value to -20 dB.
- 42 Hold probe in place as described previously.
- 43 The display on screen is V_{out} .

Displaying Vout/Vin Response on the VNA

- 44 Press the **[Display]** key.
- 45 Then select the **Data/Memory** screen key. You may need to adjust the **Reference Value**, located under the **Scale Ref** key, slightly to position the waveform at center screen.
- 46 Press marker key and position the marker to the first point that the signal is -3 dB below center screen.
- 47 Read the marker frequency measurement and record it in [Table 10](#) on page 46.
- 48 The bandwidth test passes if the frequency measurement is greater than or equal to the probe's bandwidth limit, which is 1.5 GHz.

Performance Test Record

The recommended Test Interval: 1 year / 2000 hours.

Table 10 Performance Test Record

Probe Amplifier	Test Limits	Result	Pass/Fail
Test 1. DC Input Resistance	1 M Ω \pm 3%		
Test 2. Bandwidth	\geq 1.5 GHz		

Index

Numerics

3D probe positioner, 28

A

accessories

available, 10
supplied, 8

attenuation ratio, 32

available accessories, 10

B

bandwidth, 5, 14, 32

C

cable, 6

calibration, probe, 27

CE mark, 25

channel identification rings, 8

cleaning, 22

compatibility, 7

compatible oscilloscopes, 7

D

dynamic range, 20, 32

E

ESD, 6

F

flex nose clip, 10, 11

functional test, 21

G

ground lead, 12

H

headlight, 8

I

impedance, channel input, 7

Infiniium oscilloscope, 7

InfiniiVision oscilloscope, 7

input capacitance, 32

input impedance over frequency, 36

input resistance, 32

inspecting, 22

ISM1-A, 26

K

Keysight Technologies, contacting, 23

N

N2787A 3D probe positioner, 12

O

offset range, 20

operating temperature

accessories, 11, 12

probe, 31

oscilloscope

compatibility, 7

Infiniium, 7

InfiniiVision, 7

oscilloscope compatibility, 7

output impedance, 32

P

performance test record, 46

performance verification, 37

probe

cleaning, 22

configurations, 14

handling, 24

inspecting, 22

service, 23

probe accessories, 14

probe calibration, 27

Probe Calibration dialog box, 28

probe positioner, 12

probe, inspecting, 22

PV fixture, 28

R

returning for service, 23

right angle ground, 10, 11

right-angle ground, 15, 17

rigid probe tip, 10, 11

rigid tip, 15

rigit tip, 15

S

safety information, 24

service, 23

solderable pin, 10, 11

solderable tip, 17

specifications, 31

spring ground, 11

spring probe tip, 12

supplied accessories, 8

Y

Y-lead adapter, 10, 11

Y-lead with clips, 19

Y-leads, 16, 18

